
## cf-DNA/cf-RNA Preservative Tubes Dx Cat. Dx63950

Mixing Instructions



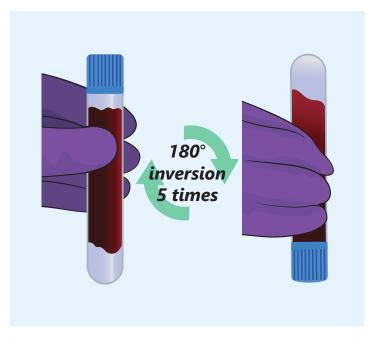

## **Norgen Biotek Corp.** 3430 Schmon Pkwy, Thorold, ON, Canada, L2V 4Y6 www.norgenbiotek.com | info@norgenbiotek.com

## **IMPORTANT!**

**Immediately** after blood is drawn into the tube, invert the tube five times (x5) to ensure that the preservative makes uniform contact with the sample.

One inversion is a complete turn of the wrist 180 degrees and back.

**DO NOT MIX** the contents of the cf-DNA/cf-RNA Tube again once this step is complete.