



Proper Blood Collection and Mixing Procedure

WARNING!

Blood must be **mixed** with the cf-DNA/cf-RNA preservative upon collection **immediately** or within **1 minute**, otherwise **hemolysis** & **blood clotting** will begin to take place.

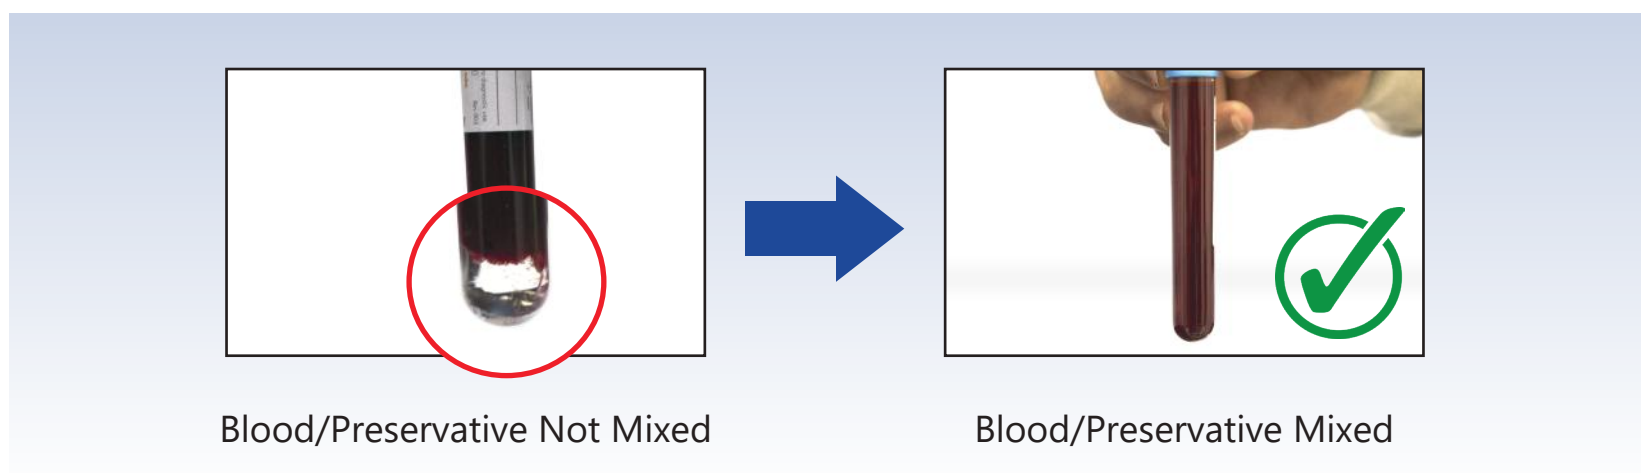

Mix Immediately or Within 1 Minute Maximum

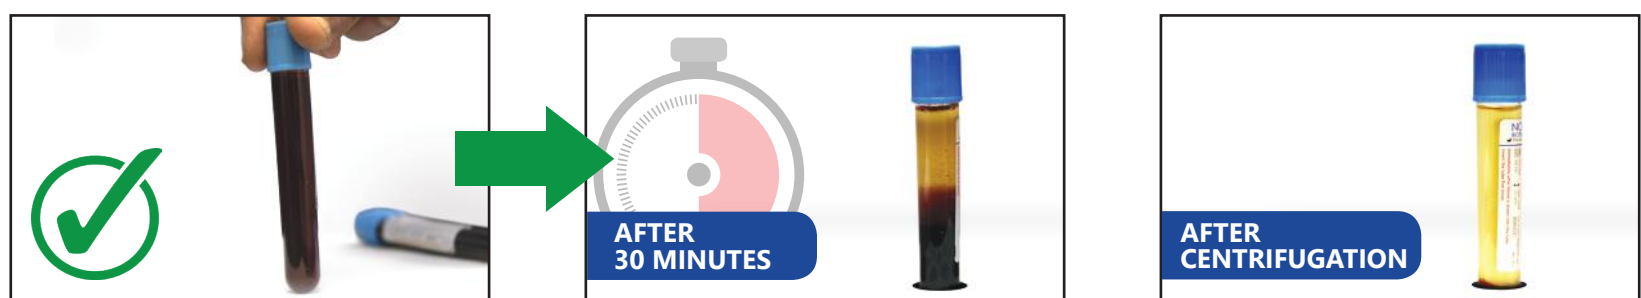

Mixing After 2 Minutes Voids Use of Product

